

ARU 700

Terminal Electrolytic Recovery


Application Range: 2.5 to 3 gallons per day (24 hours).

Typical Silver Discharge: 0.75 PPM to 3 PPM.

Application Notes:

- Replace RePAC cartridge every 300 gallons processed, or every 6 months.
- Limit collection of silver on the cathode to 6-8 pounds.
- Clean out CT-5 tank and overflow fittings every 6 months.

Typical Installation:

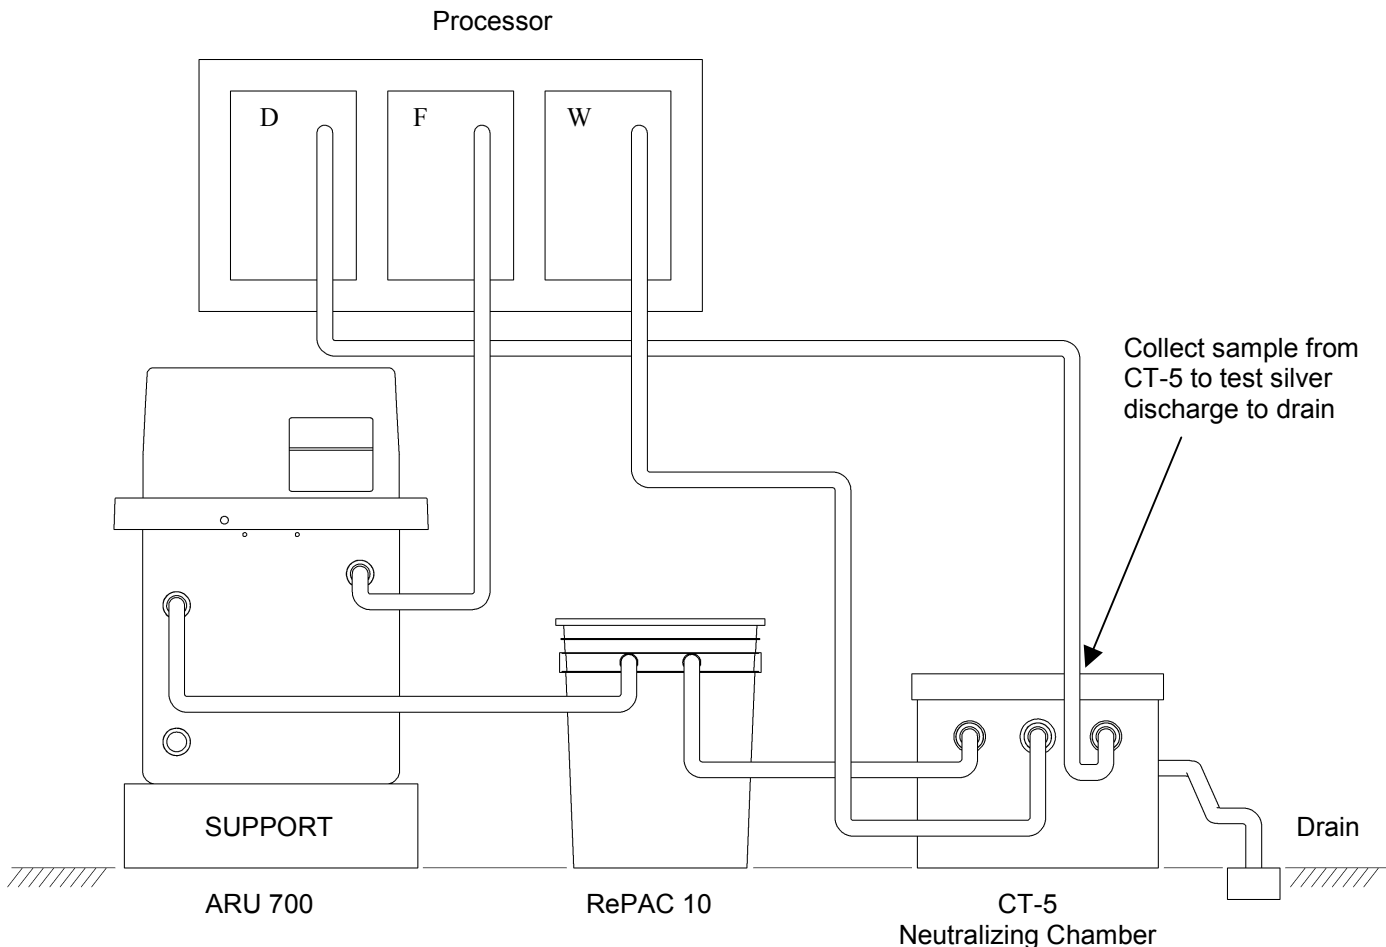

* Support must be used to raise the unit above the tailing cartridge inlet.